

Ion-Selective Electrodes for the Determination of Periodate IO_4^- Using Periodate - Tetrazolium Chloride (TTC) as an Ion-Pair and its Applications

Hamdy AB. Matter^{1,2*}, Tariq M. Ayad¹

¹ Chemistry Department, Benghazi University, El-Wahat, Libya.

² High Institute of Engineering and Technology, El-Arish, Egypt.

Received 08 / 11 / 2022; Accepted 22 / 01 / 2023

المخلص

تم تحضير، وفحص غشاء بولي (كلوريد الفينيل) (PVC) المكون من 2، 3، 5 – تري فينيل تيترازوليوم كلوريد (KIO_4 - TTC) مع رباعي فينيل بورات الصوديوم (NaTPB) كمستبعد أنيون، وثنائي أوكثيل فثالات (DOP) وثنائي أوكثيل سبيكات (DOS) كمادة ملدنة، ويعمل كقطب انتقائي لـ KIO_4 ، ولوحظ أفضل أداء للغشاء الذي يحتوي على مادة الترابط تركيبة من (KIO_4 - PVC-TTC) (5mg)، وملدن (DOP) (200mg) - PVC و NaTPB و 100mg: رباعي فينيل بورات الصوديوم: 5mg، والتي عملت بشكل جيد على مدى تركيز واسع (1.5×10^{-6} - 1.0×10^{-1} M) من (50 - 55.0) مللي فولت لكل عقد تركيزات من النشاط بين الرقم الهيدروجيني (3 - 10) pH أظهرت هذه الأقطاب الكهربائية وقت استجابة سريعًا من 5 إلى 15 ثانية، وتم استخدامها على مدى 90 صبغة مع قابلية استنساخ جيدة، ومعامل الانتقائية لـ الأيونات أحادية التكافؤ وثنائية التكافؤ تشير إلى انتقائية ممتازة لـ IO_4^- أيونات على عدد كبير من الأيونات، تم استخدام المستشعر لتحديد IO_4^- أيونات في آبار المياه في منطقتي أوجلي، وجالو بمنطقة الواحات / ليبيا وكذلك في مياه الصرف.

الكلمات المفتاحية: الأقطاب الكهربائية الانتقائية الأيونية، البير أيودات، كلوريد تترازوليوم، مياه الصرف.

Abstract

Poly (vinyl chloride) (PVC) membrane-based of 2, 3, 5 –Triphenyltetrazolium Chloride (TTC)- KIO_4 with sodium tetraphenylborate (NaTPB) as an anion excluder and dioctylphthalate (DOP) and dioctylsebacate (DOS) as plasticizer were prepared and studied as a KIO_4^- selective electrode. The best performance was observed with the membrane having the ligand (TTC KIO_4 – PVC – plasticizer (DOP) – NaTPB (sodium tetraphenylborate) composition 5: 100: 200: 5mg, respectively, which worked well over a wide concentration range (1.5×10^{-6} M – 1.0×10^{-1} M) with a Nernstian slope of 50–55.0 mV per decade of activity between pH 3 and 10.0. These electrodes showed a fast response time of 5 – 15 s and were used over a period of 90 dyes with good reproducibility. The selectivity coefficient for monovalent and divalent anions indicated excellent selectivity for IO_4^- ions over a large number of anions. The sensor has been used to determine IO_4^- ions from Ojela and Jalu /Libyan water wells and wastewater.

Keywords: Ion-selective electrodes, Periodate, Tetrazolium chloride, Wastewater.

1. INTRODUCTION

Triphenyltetrazolium chloride was used for determining iodate and periodate^[1]. Iodonitrotetrazolium chloride and tetrazolium violet were used for determining chromium spectrophotometrically^{[2],[3]}. Triphenyltetrazolium chloride was used for determined mercury in soils spectrophotometrically^[4]. 2, 3, 5-Triphenyl-2H-tetrazolium chloride was used as a reagent for sugar determination^[5]. Neotetrazolium chloride formed the ion-pair of tetrathiocyanatocobaltate (II) to determine cobalt (II) spectrophotometrically^[6]. Tetranitro-blue tetrazolium was used for determined selenium spectrophotometrically^[7]. An electrochemical sensor for determined iodate and periodate^[8]. Methylene blue was used for determining periodate and iodate spectrophotometrically^[9], periodate and iodate were determined spectrophotometrically by calculating the rates of reactions in acidic media with iodide^[10].

IrO_2 nanoparticles are grown on a glassy carbon electrode by electrodeposition method, Iodate and periodate are reduced and the electrochemical properties and electrocatalytic activity of the modified electrode are investigated^[11]. Dopamine was determined in pharmaceutical preparations based on its oxidation with (IO_4^-) using a new IO_4^- -selective electrode^[12], and (IO_4^-) oxidation constrict to the development of selective devices methods of micro-analysis in several fields like electrochemistry, spectrophotometry, chromatography, luminometry, are successful manufacturing of sensors or labeling techniques^[13]. The ion-associate of (IO_4^-) extraction balance with HCl was studied spectrophotometrically^[14]. Liquid-membrane for determining (IO_4^-) by the ion-selective electrode and its implementation to the potentiometric titration of α -diols and α -amino-alcohols occurred^[15], (IO_4^-) -selective electrode was utilized for determining tartaric acid^[16], and (IO_4^-) -sensitive ClO_4^- by the ion-selective electrode in the kinetic ultra-micro-determination of manganese (II) was used^[17]. Fluorometric analysis of (IO_4^-) based on the oxidation of 2-acetylnaphthol phenyl selenoether and application to the assay were regenerated of (IO_4^-)^[18]. The ion-selective membranes were made of PVC with ionophore porphyrin-based sensing systems and cation lipophilic as additive materials was used to

*Correspondence: Hamdy AB. Matter
hamdy.matter@uob.edu.ly

calculate (IO_4^-) concentration [19]. A method for the determination of reducing sugars in serum was studied; the sample reacted with an excess of (IO_4^-) in a flow system and the decrease in (IO_4^-) [20], and the tubular (IO_4^-) electrode for flow-injection determination of glycerol was developed [21]. Sucrose $\text{C}_{12}\text{H}_{22}\text{O}_{11}$ was determined in milk products and soft drinks by the acid hydrolysis of sucrose and lactose with the rate of the reaction of (IO_4^-) with quenched aliquots of the solution in which hydrolysis takes place [22], and used nickel (II) Schiff bases, as a neutral carrier to make ion-selective membrane electrodes for the determination of (IO_4^-) [23]. Riboflavin immobilized multi-walled carbon nanotubes amendment electrode GCE/MWCNT-RB was prepared and proved as an electrochemical selective sensor for (IO_3^-) detection [24], and oxalate was determined by the kinetic spectrophotometric method and based on it improved the effect on the oxidation of Mn (II) to MnO_4^- ; by KIO_4 [25]. IO_4^- consumption by use of an iodide-selective electrode was calculated [26]. An excited state intramolecular proton transfer (ESIPT) fluorescent probe for highly selective and ratio-metric was used for the detection of IO_4^- [27]. Iodate and IO_4^- at the microgram level were determined by a kinetic method [28].

This study used 2, 3, 5-Triphenyl-2H-tetrazolium chloride with periodate as an ion-pair sensor electrode for determining periodate by the ion selective electrode method and applied this method for determining the periodate in wells water, juices, and wastewater.

2. EXPERIMENTAL

2.1. Reagents and Materials

All chemicals were of analytical reagent grade unless otherwise stated and doubly distilled water was used throughout. Periodate KIO_4 (M. wt. = 230) was obtained from Aldrich Chem. Co., polyvinyl chloride PVC powder of Mwt~10000 (THF) tetrahydrofuran solvent 99%, inhibited by 0.025% butylate dihydroxy toluene, dioctylsebacate DOS, sodium tetraphenylborate (NaTPB) as an anion excluder, and dioctylphthalate DOP as a plasticizer with a purity of ~99%. 10^{-1} M solution of KIO_4 was prepared by dissolving 2.3 g of KIO_4 in 100 ml of (0.05 M) PO_4^{3-} buffer solution pH 7. IO_4^- ion (10^{-1} M – 10^{-6} M) solution was prepared then, dilution of the IO_4^- ion solution by 0.05 M PO_4^{3-} , buffer solution of pH 7, and 2, 3, 5 Triphenyltetrazolium chloride TTC or simply Triphenyltetrazolium chloride as a redox indicator commonly used in biochemical experiments specially to indicate cellular respiration. It is a white crystalline powder, soluble in water, ethanol and acetone but insoluble in ether.

2.2 Apparatus

All Potentiometric Apparatus at 25 ± 1 °C with an Orion pH / mV meter. A double junction Ag / AgCl reference electrode was used, and an electrode (Model 90 – 02) filled with 10% (w/v) KCl was used in the outer closet. A glass electrode (Orion 81– 02) was used for pH measurements.

2.3. Synthesis of (TTC- KIO_4) ion pair

1g of TTC was dissolved in 100 ml distilled water + 1g KIO_4 in 100 ml distilled water; white precipitate was formed.

2.4. Preparation of Membrane

Homogeneous membranes of TTC – KIO_4 ion pair were prepared by using PVC as a binder, DOP and DOS as a plasticizer and NaTPB (sodium tetraphenylborate) (anion excluder) were mixed and dissolved the membrane components in diluent THF. Then it was stirred vigorously until the result was a homogeneous syrup. After all the air bubbles were removed, it was poured into glass casting rings resting on a smooth glass plate. The solvent was evaporated at room temperature. After waiting for about 48h, a transparent membrane of about 0.5 mm thickness was obtained from which about 5 mm in diameter was cut away from the inner edge of the cyclic ring and stuck to one end of the polyethylene tube with the membrane by THF.

2.5. Potential Measurement

The membranes were equilibrated with 10^{-2} M KIO_4 solutions for two days and the potential across the membranes was measured with potential membrane used in the outer of reference electrodes in a tube; (10^{-2} M KIO_4 solution + 10^{-2} M KCl) as an internal solution. All the measurements were made at a constant temperature of 25 ± 0.1 °C. Response time was determined after the potential of one solution of 10^{-6} M KIO_4 solution became constant and similar measurements were carried out in another solution of 10–fold higher concentrations. The response time is measured as the time taken to reach an mV of 90% of the potential difference in the two following measurements. Reproducibility can be known as the deviation from the average potential value in the same four dips measurements data.

3. RESULTS AND DISCUSSION

TTC is a redox indicator commonly used in biochemical experiments specially to indicate cellular respiration. The crystalline powder (white) was soluble in water, ethanol and acetone but insoluble in ether [29].

The reaction involves (TTC) with KIO_4 ; the white precipitate was formed from the TTC- KIO_4 complex used as an ion pair in an ion-selective membrane with (NaTPB) as an anion excluder and (DOP) as a plasticizer. PVC and THF were prepared and studied as a KIO_4 -selective electrode for the calculation of the concentration of KIO_4 in water or wastewater or other samples using a calibration curve, and the time of response recorded quadrature the IUPAC recommendation [30].

An electrode membrane contains a solvent mediator (DOP) and DOS; the electrodes achieved an equilibrium response within 15 – 20 s over a whole concentration range of 1.41×10^{-6} M – 1.0×10^{-1} M. The potentials obtained must be still constant for more than 5 min, after a slow variation of data is observed. All potentials were measured periodically and the standard deviation of about 50 mV corresponding measurements was ± 0.4 mV. The lifetime of electrodes based on ion pairs in solvent polymeric membranes depends on the distribution coefficient of the ion pairs and plasticizer between the aqueous and membrane phases. Hence, the lifetime of electrodes must depend on the compositions of the solution and the measured compounds with electrodes. The results experimentally explain that the lifetime of the present electrode was about 15 weeks, the detection limit was stable, and the slope of the electrode was observed to be constant, and remained constant, during this time. The

electrochemical demeanor of the electrodes gradually degenerates after 15 weeks, which can be due to the senility of the (PVC), DOP plasticizer and ion pair (TTC) (IO_4^-) [31].

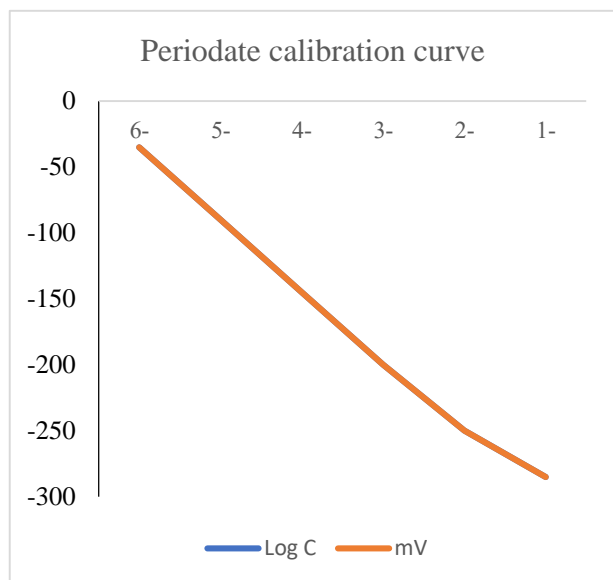


Fig. 1. The relationship between log C in the X- axis and mV in the Y- axis for IO_4^-

KIO_4 -TTC membrane contains the DOP as a plasticizer and shows linearity at the concentration range between 1.0×10^{-5} M, and 1.0×10^{-1} M a slope of about $55 \text{ mV} \pm 0.4 \text{ mV}$ per (10) decade. Hence, the membrane electrode was investigated as a KIO_4 selective electrode and all further were studied with this membrane electrode. The salts which incorporated, and which consisted of a hydrophobic cation and a lipophilic anion, e.g., (NaTPB), based on TTC- IO_4^- have proved to be beneficial in several respects [32].

Sodium tetraphenylborate (NaTPB) reduces interference by lipophilic anions in the sample by bringing about significant changes in selectivity and boosting the anion selectivity in the case of carriers with poor extraction capability and decreasing the electrical membrane resistance considerably [33,34]. When preparing the electrode without NaTPB, the sensitivity of the electrode and selectivity for KIO_4 was decreased, due to the high resistance of anions in the solution. NaTPB acts as an ion exchanger [35]; hence NaTPB was used, leading to drastic changes in the shape of the slope, and in more response, the membrane electrode becomes more selective.

The electrode potential was investigated over the pH range 2.0 – 12.0 for 1.0×10^{-3} M and 1.0×10^{-4} M of KIO_4 . The pH changed with HNO_3 acid or ammonia hydroxide solution. The potential is still stable between pH 3.0 – 9.0 (Fig. 2) and the same can act in this working range of pH of the electrode perfectly.

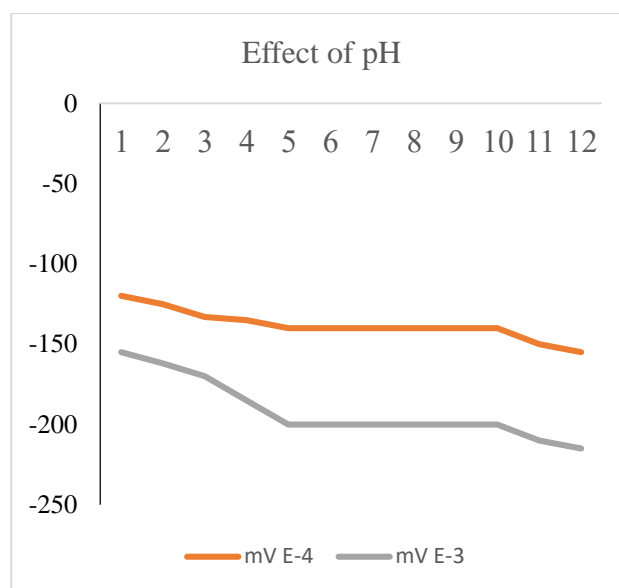


Fig.2. Effect of pH in X- axis and – mV in Y- axis at concentrations 10^{-3} M and 10^{-4} M of IO_4^-

This paper used the Matched Potential Method (MPM) to calculate the selectivity coefficients $K^{\text{Pot}} \text{IO}_4^-$ [36] at a 1.0×10^{-2} M concentration of some interfering ions. By studying interfering ions and periodate, the electrode was selective to determine KIO_4 concentration (Table 1); the reversibility of the membrane electrode which can be calculated in a similar step in the opposite direction was done. The data was placed in the sequence from high values to – low values, i.e., from 1.0×10^{-2} to 1.0×10^{-3} M concentrations of samples, and the results explained that the potentiometric response of the membrane electrodes was reciprocal; although the equilibrium values were reached at the time about (50 s) which is a longer time than that of low to – high concentrations of samples. The lifetime of a membrane or membrane electrode is nearly 2 months [37,38,39,40,41], and the reproducibility of the electrode was studied by using six similarly constructed TTC – KIO_4 electrodes under several conditions. The results explained a good Nernstian slope of about $50 \text{ mV} (\pm 0.4 \text{ mV})$ for the membrane electrode.

Table1. Selectivity coefficient data ($K^{\text{Pot}} \text{IO}_4^-$) for IO_4^- selective membrane electrode contain TTC- IO_4^- ion-pair.

Interfere	$K^{\text{Pot}} \text{IO}_4^-$	Interferes	$K^{\text{Pot}} \text{IO}_4^-$
KIO_4	2.3×10^{-5}	K_2CO_3	1.3×10^{-4}
KIO_3	2.2×10^{-5}	KHCO_3	1.4×10^{-5}
KClO_4	2.1×10^{-4}	KMnO_4	1.1×10^{-4}
KClO_3	1.2×10^{-4}	K_2CrO_4	2.3×10^{-4}
K_2SO_4	1.3×10^{-4}	$\text{K}_2\text{Cr}_2\text{O}_7$	1.2×10^{-4}
K_2SO_3	1.2×10^{-5}	KH_2PO_4	1.3×10^{-5}
KHSO_4	1.4×10^{-5}	K_3PO_4	1.4×10^{-5}
KNO_3	1.1×10^{-4}	CH_3COOK	1.1×10^{-4}
KNO_2	1.2×10^{-4}	$(\text{OH})_2(\text{CH})_2(\text{COOK})_2 \cdot 5\text{H}_2\text{O}$	1.3×10^{-4}

3.1. Application of IO₄⁻ Sensor Electrodes

Table 2: Determination of IO₄⁻ in the well water from Ojela and Jalu wells, juices, and wastewater.

Sample	Concentration (ppm)
(Water well 1)	230
(Water well 2)	23
(Water well 3)	12
Orange juice	4
Beetroot	12
Carrot juice	8

4. CONCLUSION

The TTC-IO₄⁻ membrane electrode incorporating an ion-pair can be seen in the expansion of the IO₄⁻ ion-selective electrode. The data shows that the (DOP) plasticizer electrode proved to be a good solvent mediator for electrode construction. The suggestion electrode showed high selectivity and sensitivity to IO₄⁻ ions, and a fast time response with a Nernstian slope of about 55.0 mV/decade to IO₄⁻ for a large scale of the concentration range of 1.5×10^{-6} M – 1.0×10^{-1} M. The proposed electrode revealed excellent selectivity towards IO₄⁻ and was used to determine IO₄⁻ in water, wastewater, and different juice samples which may contain IO₄⁻.

5. REFERENCES

- Kamburova, M. (1992). Triphenyltetrazolium chloride for determination of iodate and periodate. *Talanta*, 39(8), 997-1000.
- Kamburova, M. (1993). Spectrophotometric determination of chromium with iodinitrotetrazolium chloride and tetrazolium violet. *Talanta*, 40(5), 707-711.
- Kamburova, M. (1993). Iodinitrotetrazolium chloride—A new analytical reagent for determination of chromium. *Talanta*, 40(5), 725-728
- Kamburova, M. (1993). Spectrophotometric determination of mercury in soils with triphenyltetrazolium chloride. *Talanta*, 40(5), 719-723.
- Mark Jr, H. B., Backes, L. M., Pinkel, D., & Papa, L. J. (1965). 2, 3, 5-Triphenyl-2H-tetrazolium chloride as a reagent for the determination of sugar mixtures by a differential reaction-rate technique. *Talanta*, 12(1), 27-34.
- Singh, A. K., Kumar, D., & Katyal, M. (1985). Spectrophotometric determination of cobalt (II) based on the ion-pair of tetrathiocyanatocobaltate (II) with neotetrazolium chloride. *Analytica chimica acta*, 172, 303-306.
- Hawkes, W. C. (1986). Spectrophotometric determinations of traces of selenium by catalytic reduction of tetranitro blue tetrazolium. *Analytica chimica acta*, 183, 197-205.
- Chatraei, F., & Zare, H. R. (2013). Nano-scale islands of ruthenium oxide as an electrochemical sensor for iodate and periodate determination. *Materials Science and Engineering: C*, 33(2), 721-726.
- Afkhami, A., & Zarei, A. R. (2001). Spectrophotometric determination of periodate and iodate by a differential kinetic method. *Talanta*, 53(4), 815-821.
- Afkhami, A., & Zarei, A. R. (2003). Simultaneous kinetic-spectrophotometric determination of periodate–bromate and iodate–bromate mixtures using the H-point standard addition method. *Talanta*, 60(1), 63-71.
- Salimi, A., Hallaj, R., Kavosi, B., & Hagighi, B. (2010). Highly sensitive and selective amperometric sensors for nanomolar detection of iodate and periodate based on glassy carbon electrode modified with iridium oxide nanoparticles. *Analytica chimica acta*, 661 (1), 28-34.
- Montenegro, M. C. B. S. M., & Sales, M. G. F. (2000). Flow-injection analysis of dopamine in injections with a periodate-selective electrode. *Journal of pharmaceutical sciences*, 89 (7), 876-884.
- Vlessidis, A. G., & Evmiridis, N. P. (2009). Periodate oxidation and its contribution to instrumental methods of micro-analysis—A review. *Analytica chimica acta*, 652(1-2), 85-127.
- El-Shahawi, M. S. (1997). Extraction equilibrium of the ion-associate of periodate with amiloride hydrochloride and simultaneous spectrophotometric determination of periodate and iodate by liquid–liquid extraction. *Analytica chimica acta*, 356 (1), 85-91.
- Kudoh, M., Kataoka, M., & Kambara, T. (1980). Construction of a liquid-membrane type periodate ion-selective electrode and its application to the potentiometric titration of α -diols and α -amino-alcohols. *Talanta*, 27 (6), 495-498.
- Hartofylax, V. H., Efstathiou, C. E., & Hadjiioannou, T. P. (1986). Kinetic study of the tartaric acid-periodate reaction: Determination of tartaric acid using an improved periodate-selective electrode. *Microchemical Journal*, 33 (1), 9-17.
- Efstathiou, C. E., & Hadjiioannou, T. P. (1977). Use of a periodate-sensitive perchlorate ion-selective electrode in the kinetic ultramicro determination of manganese (II) by means of its catalytic effect on the periodate-acetylacetone reaction. *Talanta*, 24 (4), 270-272.
- Choi, M. G., Shin, E. J., Seo, Y., Ahn, S., & Chang, S. K. (2021). Fluorometric analysis of periodate based on the oxidation of 2-acetyl naphthol phenylselenoether: Application to the assay of regenerated periodate. *Sensors and Actuators B: Chemical*, 349, 130764.
- Guerreiro, J. R. L., Kamel, A. H., & Sales, M. G. F. (2010). FIA potentiometric system based on periodate polymeric membrane sensors for the assessment of ascorbic acid in commercial drinks. *Food chemistry*, 120 (3), 934-939.

20. Diamandis, E. P., Efstathiou, C. E., Papastathopoulos, D. S., & Hadjiioannou, T. P. (1983). Continuous-flow determination of reducing sugars in serum by reaction with periodate ions, with use of a flow-through periodate-sensitive electrode. *Microchemical Journal*, 28 (2), 227-234.
21. Conceição, M., Montenegro, B. S. M., Lima, J. L. F. C., Mattos, I. L., Neto, G. O., Gomes, J. A., & Zagatto, E. A. (1993). Development of a tubular periodate electrode for flow-injection determination of glycerol. *Talanta*, 40 (10), 1563-1568.
22. Hartofylax, V. H., Efstathiou, C. E., & Hadjiioannou, T. P. (1989). Kinetic study of the acid hydrolysis of sucrose and lactose and kinetic determination of sucrose using a periodate-selective electrode. *Analytica chimica acta*, 224, 159-168.
23. Aziz, A. A. A., & Kamel, A. H. (2010). Batch and hydrodynamic monitoring of vitamin C using novel periodate selective sensors based on a newly synthesized Ni (II)-Schiff bases complexes as a neutral receptor. *Talanta*, 80 (3), 1356-1363.
24. Nellaiappan, S., & Kumar, A. S. (2013). Selective flow injection analysis of iodate in iodized table salts by riboflavin immobilized multiwalled carbon nanotubes chemically modified electrode. *Electrochimica Acta*, 109, 59-66.
25. Hassouna, M. E. M., & Elsuccary, S. A. A. (2002). Determination of oxalate based on its enhancing effect on the oxidation of Mn (II) by periodate. *Talanta*, 56(1), 193-202.
26. Honda, S., Sudo, K., Kakehi, K., & Takiura, K. (1975). Periodate oxidation analysis of carbohydrates: Part III. Potentiometric determination of periodate consumption by use of an iodide-selective electrode. *Analytica chimica acta*, 77, 274-277.
27. Huang, C., Jia, T., Yu, C., Zhang, A., & Jia, N. (2015). An ES IPT-based fluorescent probe for highly selective and ratiometric detection of periodate. *Biosensors and Bioelectronics*, 63, 513-518.
28. Garrido, A., Silva, M., & Perez-Bendito, D. (1986). Determination of iodate and periodate at the microgram level by a kinetic method. *Analytica chimica acta*, 184, 227-234.
29. Kamburova, M. (1993). Spectrophotometric determination of mercury in soils with triphenyltetrazolium chloride. *Talanta*, 40 (5), 719-723.
30. Chen, P., Fryling, M. A., & McCreery, R. L. (1995). Electron transfer kinetics at modified carbon electrode surfaces: the role of specific surface sites. *Analytical Chemistry*, 67(18), 3115-3122.
31. Oesch, U., & Simon, W. (1980). Lifetime of neutral carrier-based ion-selective liquid-membrane electrodes. *Analytical Chemistry*, 52 (4), 692-700.
32. Morf, W. E., Kahr, G., & Simon, W. (1974). Reduction of the anion interference in neutral carrier liquid-membrane electrodes responsive to cations. *Analytical Letters*, 7 (1), 9-22.
33. Morf, W. E., & Simon, W. (1978). Ion-selective electrodes based on neutral carriers. In *Ion-selective electrodes in analytical chemistry* (pp. 211-286). Springer, Boston, MA.
34. Ammann, D., Morf, W. E., Anker, P., Meier, P. C., Pretsch, E., & Simon, W. (1983). Neutral carrier-based ion-selective electrodes. *Ion-selective electrode reviews*, 5, 3-92.
35. Meier, P. C., Morf, W. E., Läubli, M., & Simon, W. (1984). Evaluation of the optimum composition of neutral-carrier membrane electrodes with incorporated cation-exchanger sites. *Analytica chimica acta*, 156, 1-8.
36. Bakker, E., Pretsch, E., & Bühlmann, P. (2000). Selectivity of potentiometric ion sensors. *Analytical chemistry*, 72 (6), 1127-1133.
37. Srivastava, S. K., Gupta, V. K., & Jain, S. (1996). PVC-based 2, 2, 2-cryptand sensor for zinc ions. *Analytical chemistry*, 68 (7), 1272-1275.
38. Gupta, V. K., Goyal, R. N., & Sharma, R. A. (2009). Novel PVC membrane-based alizarin sensor and its application; determination of vanadium, zirconium and molybdenum. *Int J Electrochem Sci*, 4 (1), 156-172.
39. Pleniceanu, M., Preda, M., Muresan, N., & Simoiu, L. (1996). New liquid-membrane electrodes used for the determination of copper and nickel. *Analytical Letters*, 29 (9), 1485-1496.
40. Teltig-Diaz, M., & Bakker, E. (2001). Effect of lipophilic ion-exchanger leaching on the detection limit of carrier-based ion-selective electrodes. *Analytical chemistry*, 73 (22), 5582-5589.
41. Matter, H. A. (2013). PVC membrane based of 2, 3, 5-Triphenyltetrazolium Chloride (TTC) and 2, 4, 5-Triphenyltetrazolium Formazan (TTF) for determination Ba²⁺ and its application of crystal growth.